

Original article (short communication)

Technical application and the level of discomfort associated with an intramuscular electromyographic investigation into gluteus minimus and gluteus medius.

Adam I. Semciw,¹ Tania Pizzari¹ & Rodney A. Green²

Department of Physiotherapy¹ & Department of Rural Human Biosciences², La Trobe University, Australia

Corresponding Author

Adam Semciw

Department of Physiotherapy, La Trobe University, Bundoora, Victoria, Australia. 3086

Telephone +613 9479 5851

Email: adam.semciw@gmail.com

Acknowledgements

Sports Medicine Australia Research Foundation for assistance with participant reimbursement.

Abstract (181/250 words)

Our current theoretical understanding of gluteus minimus (GMin) and gluteus medius (GMed) function is primarily based on cadaveric studies and biomechanical modelling. There is an absence of electromyographic (EMG) research that aims to verify this understanding, particularly in relation to the potentially unique functional roles of structurally distinct segments within GMin (anterior and posterior) and GMed (anterior, middle and posterior). The aim of this paper is to provide a comprehensive technical description for inserting intramuscular EMG electrodes into uniquely oriented segments of GMin and GMed; and to **report** the levels of discomfort associated with gluteal intramuscular electrode insertions. Fifteen healthy volunteers took part in a series of walking trials after intramuscular EMG electrodes were inserted into segments of GMin (x2) and GMed (x3) according to previously verified guidelines. Visual analogue scores following walking trials at comfortable and fast speed indicate that discomfort levels associated with these insertions were low (2.4 ± 1.4 and 1.6 ± 0.7 respectively). The technical descriptions and illustrations provided in this paper will allow trained intramuscular electromyographers to insert electrodes into these muscle segments with confidence.

Keywords

Electromyography; buttocks; hip; gluteal; pain measurement.

1 **Introduction**

2 Gluteus medius (GMed) and minimus (GMin) have commonly been described in anatomical
3 studies as having three (anterior, middle and posterior) and two (anterior and posterior) segments
4 respectively with uniquely oriented fibres [1], supporting previous descriptions of functional
5 differentiation within these muscles [2]. However, the ability of these segments to function
6 independently and their role in function and dysfunction at the hip joint has not been established
7 due to a paucity of electromyographic (EMG) studies [1, 3]. This lack of research is largely due
8 to the technical expertise required to insert intramuscular needles into relevant segments of these
9 muscles, particularly given the proximity of posterior GMin to the superior gluteal neurovascular
10 bundle (NVB) [4], and the perceived pain, discomfort or anxiety that may be associated with fine
11 wire electrode insertions [5]. It is only recently that guidelines for electrode placement have been
12 validated in cadaveric specimens [3]. The aim of this paper was to provide a comprehensive
13 description of fine wire electrode insertions in segments of GMed and GMin *in-vivo* and to
14 report participant discomfort levels.

15

16 **Methods**

17 Approval was obtained from the University Human Ethics Committee to recruit 15 healthy
18 young adults (9 male, 6 female, mean age 22.5 years) for this study.

19

20 Bipolar intramuscular electrodes were prepared from two stainless steel, Teflon[®] coated wires
21 (A-M Systems, Washington, USA) according to the method of Basmajian and Stecko [6], and
22 inserted into a 23 gauge hypodermic needle. Needle (and wire) lengths were 5cm (20cm) for

23 GMed anterior and GMed middle, 7cm (20cm) for GMed posterior and GMin anterior and 9cm
24 (25cm) for GMin posterior. After manufacture, electrodes were sterilized in an autoclave.

25

26 For all measurements and electrode insertions subjects were placed in a side lying position on a
27 plinth, with hips and knees in 45° flexion, and pillow between the knees for comfort. This allows
28 for greatest access to all insertion sites without having to change positions. Electrode insertions
29 guidelines were developed with reference to real time ultrasound (RTUS) imaging *in-vivo*;
30 anatomical texts and papers and examination of cadaver specimens as described previously (Fig.
31 1) [3].

32

33 *Insert Figure 1 here*

34

35 RTUS imaging was used to determine the location of each segment, the path of the needle and
36 the depth of the insertion. Ultrasound imaging has been previously reported as a valid method for
37 judging the depth of electrode insertions into a desired muscle belly [7]. Color Doppler was used
38 for viewing the NVB prior to posterior GMin insertions (Fig. 2B). The electromyographer stood
39 posterior to the participant and the RTUS transducer was aligned in the transverse plane, and
40 placed slightly anterior to the insertion site. A sterile environment was maintained around
41 electrode insertion sites through the use of sterile gloves, cleansing of the insertion site and
42 RTUS transducer with an alcohol swab and application of sterile ultrasound gel. The insertion
43 path was then scanned to ensure that all relevant muscles, fascial and bony planes and NVBs at
44 each site were identified prior to insertion. The investigator inserted the wire and needle unit

45 until the tip of the needle was observed on the RTUS monitor to be resting in the desired muscle
46 belly.

47

48 Electrodes were inserted from anterior to posterior (see sequence below) to avoid subsequent
49 displacement of previously inserted electrodes. Insertion paths for each of the electrodes as
50 visualized on RTUS for GMed and GMin are illustrated in Figure 2. Technical notes regarding
51 insertion paths are described in Table 1.

52

53 *Insert Figure 2 here*

54

55 *Insert Table 1 here*

56

57 Following insertions, wires were taped to the skin and connected to the EMG recording
58 apparatus. Participants then completed a series walking trials (6 x comfortable walking speed, 6
59 x fast walking speed) along a 9m walkway. After each series of trials they were asked to rate
60 their level of discomfort on a visual analogue scale (VAS) of 0-10 where 0 = no discomfort and
61 10 = maximum possible discomfort. Discomfort data were averaged for each set of comfortable
62 and fast walking trials. Finally participants completed a series of 18 maximum voluntary
63 isometric contraction (MVIC) trials [8] for amplitude normalization purposes.

64

65 **Results**

66 Electrode insertions were completed as described for all 15 participants. There were no adverse
67 reactions during the insertion of electrodes although some subjects experienced transient light-

68 headedness when they first stood up after insertions. Mean discomfort scores (\pm standard
69 deviation) were 2.4 ± 1.4 and 1.6 ± 0.7 on the VAS for normal and fast walking trials
70 respectively.

71
72 Up to 2 - 4 cm of 'electrode sliding' (drawing more of the external wire length into the muscle)
73 was noted during dynamic and static manoeuvres. However, loss of data due to electrode
74 dislodgment only occurred in 1 of the 15 participants (6.7%) for GMin posterior and GMed
75 anterior segments.

76

77 **Discussion**

78 Intramuscular electrodes were successfully located in the three segments of GMed and two
79 segments of GMin previously verified in a cadaveric study [3]. Very few electrodes were
80 displaced during walking trials, adverse events were minor and participants experienced
81 relatively low levels of discomfort. The needle and wire lengths used were suitable for the
82 sample of young active participants in this study. Alternative wire and needle lengths may be
83 considered for other populations.

84

85 It has been over thirty years since EMG research was reported on GMin [9]. Processing and
86 analysis techniques have advanced since then, and there are now cadaverically verified
87 guidelines for assessing the function of multiple GMin segments [3]. Similarly, prior research
88 into unique regions of GMed are based on unverified electrode insertion guidelines [2]. As a
89 consequence, our theoretical understanding of segmental GMed function, and the function of

90 GMin is principally based on inferences from cadaveric studies and biomechanical modelling
91 [1].

92

93 This study aimed to address the paucity of segmental GMin and GMed EMG research by
94 providing a comprehensive technical guide (see Table 1 and Fig. 1 and 2) for inserting EMG
95 electrodes into segments of GMin (x2) and GMed (x3). Secondly, we have reported the level of
96 discomfort associated with gluteal insertions. The minor discomfort levels are not expected to
97 alter the recruitment patterns in these muscles [10, 11], and may be referred to in order to
98 facilitate participant recruitment, ethical approval or grant applications associated with
99 intramuscular EMG research for these muscles.

100

101 **Conflict of interest**

102 None declared.

References

1. Flack NAMS, Nicholson HD, Woodley SJ. A review of the anatomy of the hip abductor muscles, gluteus medius, gluteus minimus, and tensor fascia lata. *Clin Anat* 2012; 25(6): 697-708.
2. Soderberg GL, Dostal WF. Electromyographic study of three parts of the gluteus medius muscle during functional activities. *Phys Ther* 1978; 58(6): 691-6.
3. Semciw AI, Green RA, Pizzari T, Briggs C. Verification of a standardized method for inserting intramuscular EMG electrodes into uniquely oriented segments of gluteus minimus and gluteus medius. *Clin Anat* 2012. <http://dx.doi.org/10.1002/ca.22055>.
4. Akita K, Sakamoto H, Sato T. Origin, course and distribution of the superior gluteal nerve. *Cells Tissues Organs* 1994; 149(3): 225-230.
5. Young CC, Rose SE, Biden EN, Wyatt MP, Sutherland DH. The effect of surface and internal electrodes on the gait of children with cerebral palsy, spastic diplegic type. *J Orthop Res* 1989; 7(5): 732-737.
6. Basmajian JV, Stecko G. A new bipolar electrode for electromyography. *J Appl Physiol* 1962; 17: 849.
7. Hodges PW, Kippers V, Richardson CA. Validation of a technique for accurate fine-wire electrode placement into posterior gluteus medius using real-time ultrasound guidance. *Electromyogr Clin Neurophysiol* 1997; 37(1): 39-47.
8. Semciw AI, Pizzari T, Green RA. Intramuscular EMG placement for two segments of gluteus minimus and three segments of gluteus medius with unique orientation and function. *J Sci Med Sport* 2011; 14(7): S189.

9. Wilson GL, Capen EK, Stubbs NB. A fine-wire electromyographic investigation of the gluteus minimus and gluteus medius muscles. *Res Q* 1976; 47(4): 824-8.
10. Jacobson WC, Gabel RH, Brand RA. Insertion of fine-wire electrodes does not alter EMG patterns in normal adults. *Gait Posture* 1995; 3(1): 59-63.
11. Jacobson WC, Gabel RH, Brand RA. Surface vs. fine-wire electrode ensemble-averaged signals during gait. *J Electromyogr Kinesiol* 1995; 5(1): 37-44.
12. Moore KL, Dalley AF, Agur AMR. *Clinically Oriented Anatomy*. Philadelphia: Lippincott Williams and Wilkins; 2010. p. 578, Fig 5.46D.

Table 1

Technical notes for gluteus minimus and gluteus medius intramuscular EMG insertions.

Muscle	Segment	Order of insertion	Depth	Notes
GMin	Anterior	2	Deep to GA and GMed anterior	GMin has a hyper-echoic superficial tendon
	Posterior	3	Deep to GMax and GMed	Must use color Doppler to view safe path adjacent to NVB. May require slight movement away from marked insertion sight
GMed	Anterior	1	Deep to GA	Located superior to the belly of TFL, which does not reach the iliac crest
	Middle	4	Deep to GA	Occasionally deep to some GMax fibers
	Posterior	5	Deep to GMax	An intramuscular tendon appears as a hyper-echoic fascial plane within the posterior GMed muscle belly


GA, gluteal aponeurosis; GMax, gluteus maximus; GMed, gluteus medius; GMin, gluteus minimus; NVB, superior gluteal neurovascular bundle; TFL, tensor fascia lata.

Illustrations


Fig. 1. Location of insertion sites for gluteus medius (A) and gluteus minimus (B) segments.

Gluteus medius measurements are proportions of the length along the iliac crest from anterior (ASIS) to posterior (PSIS) superior iliac spines. GMin measurements are proportions of a direct line from the ASIS to PSIS. All insertions sites are 3cm inferior to the measured point along a line directed towards the apex of the greater trochanter (GT). Fig. 1 has been **modified with permission from [12]**.

Fig. 2: Transverse RTUS images *in-vivo* taken with a 7.5 MHz linear transducer of needle insertions into anterior (A) and posterior (B, C) GMin; as well as anterior (D), middle (E) and posterior (F) GMed. Doppler imaging is used to view the NVB (B) prior to needle insertion into posterior GMin (C). GMax, gluteus maximus; GMed, gluteus medius; GMin, gluteus minimus; IT, intramuscular tendon; N, needle; NVB, superior gluteal neurovascular bundle.

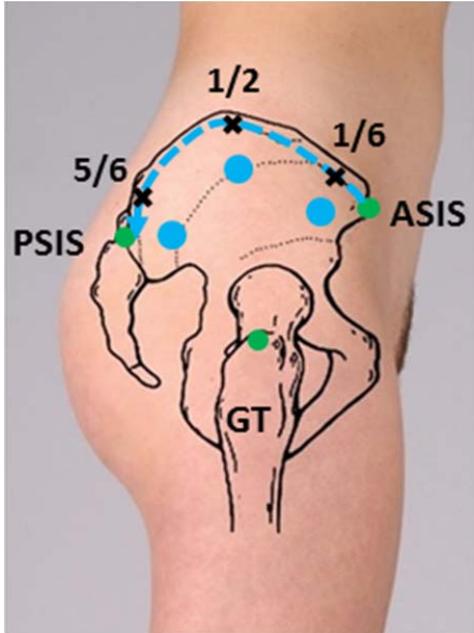

A Gluteus medius

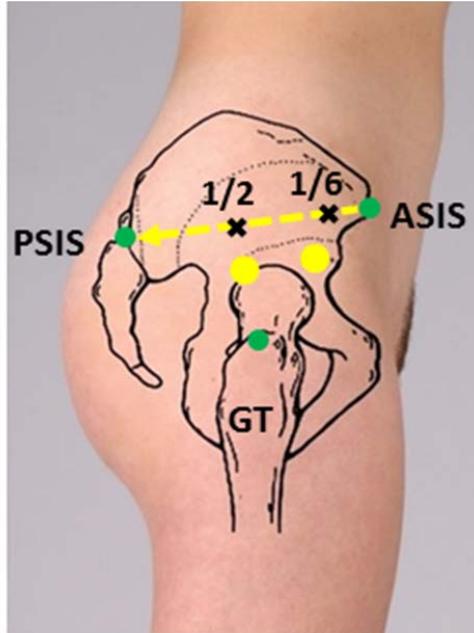

B Gluteus minimus

